



अखिल भारतीय आयुर्विज्ञान संस्थान, गोरखपुर All India Institute of Medical Sciences, Gorakhpur

(स्वास्थ्य एवं परिवार कल्याण मंत्रालय भारत सरकार द्वारा स्थापित एक स्वायत्त निकाय)
(An autonomous organization under the Ministry of Health & Family Welfare, Govt. of India)


Comp 5054

AIIMSGKP/EW/202526/679(i)

18/08/2026

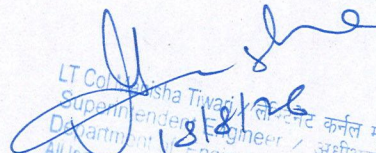
Corrigendum

Detailed specification attached for quotation notice Comp – 5054, Ref No
AIIMS/GKP/EW/679 dt 14/08/2026 for Drug Cart & Cardiac Table


18/8/26.
LT Col Manisha Tiwari / लेफ्टिनेंट कर्नल मनीषा तिवारी
Superintendent Engineer / अधीक्षक अभियंता
Department of Engineering / इंजीनियरिंग विभाग
All India Institute of Medical Sciences, Gorakhpur-273008
अखिल भारतीय आयुर्विज्ञान संस्थान, गोरखपुर-273008

Sl. No	Technical Specification	Committee observation
1	Emergency cart constructed of SS 304/aluminum and high density resin.	✓
2	Defibrillator shelf with monitor straps, glove dispenser, sharp container, oxygen cylinder cradle, IV pole, cardiac chest board, writing surface.	✓
3	Clear plastic/ABS plastic overlay for top cap.	✓
4	Push handle built in to the end panel for smooth and stable movement.	✓
5	Pullout writing surface top.	✓
6	Cart should be light, sturdy and scratch resistant.	✓
7	All drawers should be lockable	✓
8	Should have minimum of five drawers with adjustable/fixed dividers.	✓
9	Should have side bin discarding syringes and gloves.	✓
10	Lockable Castor should not be less than 5" diameter to facilitate quiet and easy maneuverability, dust-prevention, flexible transportation	✓
11	Size should be: Height up to top: 90 to 100 cms (excluding castors up to top cap) Length of base - 60-70 cms Depth/ Width: 45 - 55 cms Width and depth should be good enough to accommodate the necessary items	✓
12	Base should not be less than 60 to 70 cm	✓
13	Width and depth should be good enough to accommodate the necessary items	✓
	Comments from Committee-	Recommend for acceptance as per given Technical Specification

Drug cart


 LT Col. Asha Tiwari / लेफ्ट कर्नल मनीषा तिवारी
 Superintendent Engineer / अधीक्षक अभियंता
 Department of Engineering / इंजीनियरिंग विभाग
 All India Institute of Medical Sciences, Gorakhpur-273008
 अखिल भारतीय आयुर्विज्ञान संस्थान, गोरखपुर-273008

Sl No.	Technical Specification	Match	Mismatch
1	Should have anti-scratch, good surface finish ABS Laminated top having dimension 740-780 mm Lx 440-480 mm W approximately with +/-5% tolerance	✓	
2	Table top height can be adjusted with the help of operating lever which activates the gas spring. Adjustable from 760 to 1050 mm ($\pm 5\%$)	✓	
3	Base frame should be made of ERW round tube with 50.8 mm dia and 1.6 mm thickness. Housing should be made of aluminum extruded inner and outer tubes. Handle for gas spring made of MS sheet metal of Section 74 mm $\times$ 115mm with 3 mm thick Handle with CRCA material making strong lever and providing wider area for grip	✓	
4	Castors : High endurance anti-static, Plastic injection molded castors are provided of $\phi 50$ mm powder coating should be Bacteriostatic and thermosetting epoxy polyester, formulated to fulfill the requirements for bacterial protection.	✓	
5	Safe working Load : 20Kg or more	✓	
TECHNICAL STATUS		Comments received for the Department	

Cardiac Table

LT Col Manisha Tiwari / लेफ्टिनेंट कर्नल मनीषा तिवारी
 Superintendent Engineer / अभियंता सुपरीन्टेन्डेंट
 Department of Engineering / अभियंता विभाग
 All India Institute of Medical Sciences, Gorakhpur-273008
 अखिल भारत आयुर्वेदज्ञान संस्थान, गोरखपुर-273008